WIDEX **MENU**™

THE CHOICE IS YOURS

USER INSTRUCTIONS

THE MENU™ SERIES

ME-CIC/IIC-TR • ME-CIC/IIC model
Completely-in-canal/Invisible-in-canal

WIDEX®

HIGH DEFINITION HEARING

YOUR WIDEX HEARING AID

(To be filled out by the hearing care professional)

☐ **MENU3**
☐ **MENU5**
☐ **MENU10**

Date: _____

Battery size: 10

Vent: ☐ **Short**
☐ **Full length**
☐ **None**

Programs:

☒ **Master**
☐ **Music**
☐ **TV**
☐ **Standard**
☐ **Acclimatisation**
☐ **Audibility Extender**
☐ **Zen**

CONTENTS

DESCRIPTION OF THE HEARING AID 4
Acoustic indicators 7
The battery 8
Inserting the battery 8
Low battery indication 10
Turning the hearing aid on and off 11
Right/left identification 12
Positioning the hearing aid 13
Removing the hearing aid 15
Volume adjustment 16
Listening programs 17
Switching between the listening programs 20
CLEANING 21
The hearing aid 22
The sound outlet 24
The relief vent 25
The microphone opening 26
NANOCARE WAX GUARD 27
Changing the NanoCare wax guard 28
ACCESSORIES 31
IN CASE OF MALFUNCTION 32
CARING FOR YOUR HEARING AID 34
WARNINGS 35
ADVICE 39
SYMBOLS 41

DESCRIPTION OF THE HEARING AID

1. **Microphone opening**
2. **Battery drawer**
3. **Nail grip**
4. **On/off function**
5. **Sound outlet**
6. **NanoCare wax guard**
7. **Extraction cord**
8. **Relief vent** (short)
9. **Relief vent** (full length)

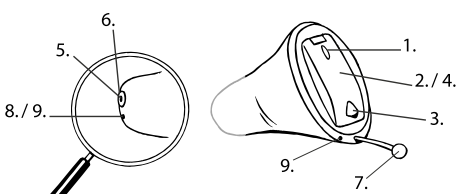

Another example of how a full length vent may be positioned.



If you need help to identify the serial number (usually six or seven digits) on the product, please contact your hearing care professional.

Your hearing aid may be provided with a listening program called Zen. It makes musical tones (and sometimes a rushing noise) in the background. These sounds are shaped according to your hearing loss.

On page 2 of this booklet your hearing care professional can indicate the type of vent used in your hearing aid, if any.

WARNING

This booklet contains important information and instructions. Please read this booklet carefully before you start using the hearing aid.

NOTE

Your hearing aid and accessories may not look exactly as illustrated in this booklet. We also reserve the right to make any changes considered necessary.

Intended use

The hearing aids are intended as air conduction amplification devices to be used in everyday listening environments. The hearing aids may be provided with the Zen program intended to provide a relaxing sound background (i.e. music/noise source) for adults who desire to listen to such a background in quiet.

Indications for use

The devices are indicated for individuals with a range of hearing loss severity from minimal (10 dB HL) to moderately severe (75 dB HL) and all hearing loss configurations.

They are to be programmed by licensed hearing care professionals (audiologists, hearing aid specialists, otolaryngologists) who are trained in hearing (re)habilitation.

Acoustic indicators

The hearing aid may be set to produce a signal to indicate the use of certain functions. The signal may be tones (SmartTone) or a spoken message (SmartSpeak)*. The signal can also be deactivated.

Functions	**Default settings**	**Other settings**
Adjusting volume via remote control	**Tone**	Off
Confirming RC program key use	**Clicking sound**	Off
Changing program via remote control	**Tones**	Message/off
Starting up the hearing aid	**Tone**	Message/off
Warning about low battery	**4 tones**	Message/off
Service reminder	**Off**	Message

** SmartSpeak not available as a standard feature*

The battery

We recommend **zinc-air batteries.** Use a **size 10** battery for the hearing aid.

To obtain replacement batteries, please consult your hearing care professional. It is important to take note of the expiry date and the recommendations on the battery pack regarding disposal of used batteries. Otherwise there is a risk that the battery life may be reduced.

Inserting the battery

Before inserting a new battery into the hearing aid, remember to remove the adhesive tab. Once the tab has been removed, the battery will start functioning after a few seconds.

CAUTION

Do not use batteries if there is a sticky residue from the tab or other unwanted substance, as this can cause the hearing aid to malfunction.



Use the nail grip to open the battery drawer. Do not press the battery drawer beyond the open position.

Place the battery in the drawer so that the small plus (+) sign on the battery is visible when you hold the hearing aid as shown.

You can use the battery magnet provided to steer the battery into place.

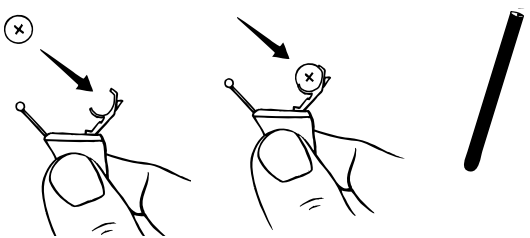

If the battery drawer does not close easily, the battery is incorrectly inserted.

When changing battery, it is a good idea to hold the hearing aid over a table.

Low battery indication

An acoustic indicator will sound when the battery is nearly exhausted, unless this function has been disabled (see page 7). We recommend that you always have a spare battery with you.

WARNING

Never leave an exhausted battery in the hearing aid. Exhausted batteries may leak, damaging the hearing aid.

WARNING

Your hearing aid may stop functioning, for instance if the battery is exhausted. You should be aware of this possibility, in particular when you are in traffic or are otherwise dependent on warning signals.

Turning the hearing aid on and off

The battery drawer of the hearing aid also functions as the on/off switch.



Close the battery drawer to turn on the hearing aid. An acoustic indicator will indicate that the hearing aid has been switched on unless this function has been disabled.



Open the battery drawer to turn off the hearing aid.

Please remember to turn off the hearing aid when it is not in use. Remove the battery if the hearing aid will not be used for several days.

Right/left identification



Your hearing aids will be marked with a red Widex logo for the right ear and a blue logo for the left ear, or they may have a red or a blue shell, respectively. The arrow shows the position of the logo.

Positioning the hearing aid



Close the battery drawer completely.



Hold your hearing aid by the extraction cord with your thumb and forefinger. Slowly guide the hearing aid into your ear canal until you feel resistance.



Let go of the extraction cord and use the tip of your forefinger to gently push the hearing aid into your ear until it rests comfortably in your canal.

To help position the hearing aid properly you could pull the outer ear backwards and upwards with the opposite hand.

If your hearing aid does not fit or sit properly, causing discomfort, irritation, redness or the like, contact your hearing care professional.

Removing the hearing aid



Gently pull the extraction cord with your thumb and forefinger.

If it is difficult, you can try to move the hearing aid carefully from side to side while pulling the extraction cord. It may also help to pull the outer ear backwards and upwards with the opposite hand.

Volume adjustment

The hearing aid volume is adjusted automatically in accordance with your sound environment.

If you have a remote control, you can also adjust the volume manually or mute your hearing aid. Any adjustment of the volume setting will be cancelled when your hearing aid is turned off, or when you change program.

If you have a remote control, please also refer to the user instructions for this.

To mute the hearing aid with a remote control:
Keep pressing the volume down key on the remote control after the long beep-tone has sounded and until it stops. Pressing one of the volume keys briefly will bring back the sound.

WARNING

If the volume in the hearing aid is generally too loud or too weak, or the reproduced sounds are distorted, or if you would like any further information, consult your hearing care professional.

Listening programs

By default, your hearing aid contains a Master program. With a remote control you have the option of an extra program, and a number of supplementary programs can also be made available. If this solution is chosen, you can have up to five programs.

Master	All the automatic functions work to ensure comfort in all listening situations
Music	For listening to music
TV	For listening to the TV
Standard	All the automatic functions work to ensure audibility and speech understanding in all listening situations
Acclimatisation	This program has the same features as the Master program but provides slightly less amplification
Audibility Extender*	Makes high-frequency sounds audible
Zen*	Generates different kinds of tones.

* *Available separately*

If your needs change over time, the combination of listening programs can be altered.

Zen program

Your hearing aid may be provided with a unique optional listening program called Zen. It makes musical tones (and sometimes a rushing noise) in the background. These sounds are shaped according to your hearing loss. The Zen program may be used alone (without amplification) in quiet when you are not required to hear surrounding sounds. Or, it may be used with the Master program so both the surrounding sounds and the generated sounds (fractal tones and noise) are heard together.

CAUTION

Use of the different Zen programs may interfere with hearing surrounding sounds including speech. The programs should not be used when hearing such sounds is important. Switch the hearing aid to a non-Zen program in those situations.

CAUTION

If you perceive a decrease in loudness, tolerance of sounds, speech not as clear, or worsening tinnitus, contact your hearing care professional.

Benefits

The Zen program may provide a relaxing listening background for some people. When the Zen program is used in a tinnitus management program, its wearer may experience some relief from tinnitus.

Indications for use

The Zen program is intended to provide a relaxing sound background (i.e., music/noise source) for adults who desire to listen to such a background in quiet. It may be used as a sound therapy tool in a tinnitus treatment program that is prescribed by a hearing care professional (audiologists, hearing aid specialists, otolaryngologists) who is trained in tinnitus management.

Directions for use

Because of the unique ways in which Zen is programmed in your hearing aid, please follow the recommendations of your hearing healthcare professionals as to how to use the program, when to use the program and/or how long to use the program.

Switching between the listening programs

To change programs via the remote control, press the program key briefly. Each time you switch to another program, an acoustic indicator will sound unless this function has been disabled.

Program 1: One short beep or message

Program 2: Two short beeps or message

Program 3: Three short beeps or message
Program 4: One long and one short beep or message
Program 5: One long and two short beeps or message

CLEANING

The following cleaning accessories are available for cleaning the hearing aid. Ask your hearing care professional which accessories you need.

1. **Brush**
2. **Cloth**
3. **Wax removing tool with a short and a long end**
4. **Long wax removing tool**

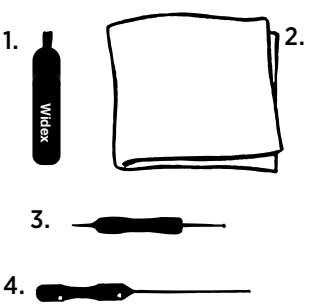

Contact your hearing care professional if you need additional supplies of cleaning accessories.

The hearing aid

It is very important for the hearing aid's performance that it is kept free from earwax and dirt.



Clean your hearing aid daily with the soft cloth to keep it dry and clean of earwax or dirt.

WARNING

Never clean the hearing aid with water or cleaning solutions, as this may cause it to malfunction.



When the hearing aid is not in use, keep it in a warm, dry place with the battery drawer open, to ventilate the hearing aid and allow it to dry.

We recommend that every time you take the hearing aid out of your ear, you inspect the sound outlet, the microphone opening in the battery drawer and the relief vent opening to ensure that no wax or dirt has gathered there.

Below is an example of how the sound outlet, relief vent and microphone opening may be positioned in a hearing aid provided with a short vent and a full length vent, respectively.

1. **Sound outlet**
2. **Relief vent** (short)
3. **Microphone opening**

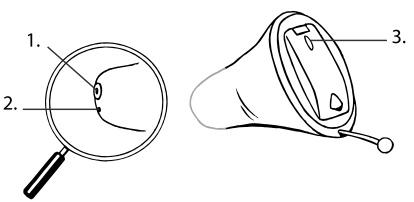

1. **Sound outlet**
2. **Relief vent** (full length, outlet)
3. **Relief vent** (full length, inlet)
4. **Microphone opening**

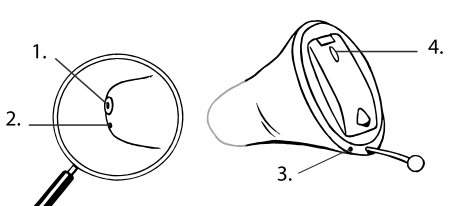

The sound outlet

It is important that the sound outlet is not blocked by earwax. If it is blocked, do as follows:



Remove any visible earwax from around the sound outlet with the small brush or cloth. Do not attempt to clean the wax guard.

If the sound outlet is still blocked, you should change the wax guard (see pages 27-30).

WARNING

If you cannot clean the sound outlet completely, you should contact your hearing care professional. Do not insert anything into the sound outlet, as this could damage the hearing aid.

The relief vent

If earwax has accumulated in and/or around the relief vent opening, do as follows:



Short vent:
Clean any earwax from the vent as far as the long end of wax removing tool no. 3 can reach.

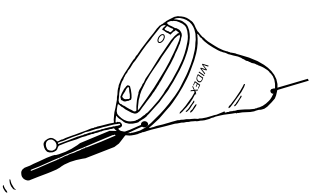

Full length vent:
Clean any earwax from the vent by passing the long wax removing tool (no. 4) all the way through the vent.

WARNING

It is important for the performance of the hearing aid that the relief vent is never blocked. Make it a habit to clean the relief vent every day! In rare cases so much earwax can accumulate in the relief vent that the hearing aid sound is affected. In that case you should see your hearing care professional.

The microphone opening

If dirt or earwax has gathered around the microphone opening on the hearing aid front, do as follows:

Open the battery drawer and remove the battery.

Turn the hearing aid so the open battery drawer is facing downwards.



Guide the short end of wax removing tool no. 3 through the microphone opening on the battery drawer from the inside as illustrated.

WARNING

If you suspect that earwax or dirt has migrated through the microphone opening and into the actual microphone inside the hearing aid, contact your hearing care professional. Do not insert anything into the actual microphone.

NANOCARE WAX GUARD

The NanoCare wax guard helps to protect the hearing aid against earwax. Always use NanoCare wax guards with your hearing aid. Otherwise the warranty for your hearing aid will be void.

The NanoCare wax guard consists of the following parts:

1. **Holder**
2. **Removal hook**
3. **Wax guard**

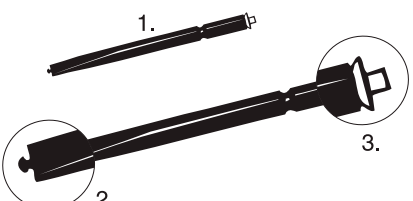

CAUTION

The wax guard is disposable and for one-time use only. Do **not** attempt to clean or reuse a wax guard. This could damage your hearing aid and/or cause the wax guard to become dislodged in your ear.

Changing the NanoCare wax guard

Insert the removal hook into the used wax guard placed in the sound outlet. Pull the wax guard straight out.

1. **Vent opening**
2. **Sound outlet**
3. **Used wax guard**

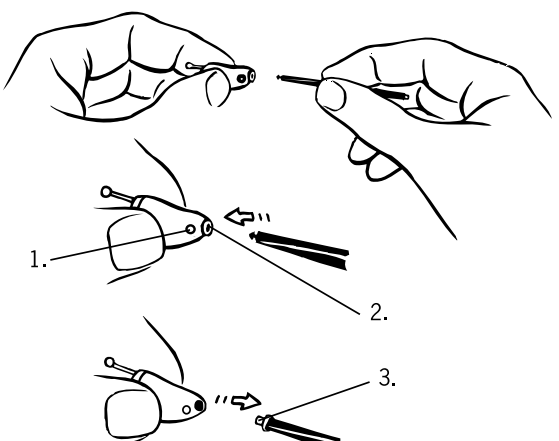

Turn the holder around so that the new wax guard is in position to be inserted.



Insert the holder into the opening of the sound outlet and gently press the wax guard into the opening.



Then pull the holder straight out.

The new wax guard will automatically detach from the holder. Press the hearing aid gently against a flat surface to ensure that the wax guard remains in place.



Discard the holder with the used wax guard.

The frequency with which the NanoCare wax guard should be changed varies from one individual to another.

If you have any questions regarding your NanoCare wax guard, please contact your hearing care professional.

WARNING

If the wax guard fits loosely, discard it and insert another. If the wax guard becomes dislodged from the hearing aid while in the ear canal, please contact your physician. Do not try to remove the wax guard from your ear canal yourself.

ACCESSORIES



Remote control
A remote control gives you a number of additional options.

For help in determining whether you could benefit from a remote control, please consult your hearing care professional.

IN CASE OF MALFUNCTION

The following pages contain some quick advice on what to do if your hearing aid stops working or performs unsatisfactorily. If the problems persist, contact your hearing care professional for assistance.

Problem	Possible cause	Solution
The hearing aid is completely silent	The hearing aid is not turned on	Make sure the battery drawer is closed
	The battery does not work	Insert a new battery in the hearing aid battery drawer
	The sound outlet is blocked	See page 24
	The microphone opening is blocked	See page 26
The hearing aid volume is not powerful enough	The battery is nearly exhausted	Insert a new battery in the hearing aid battery drawer
	The sound outlet is blocked	See page 24
	Your ear is blocked by earwax	Contact your ENT doctor/physician
	Your hearing may have changed	Contact your hearing care professional

Problem	Possible cause	Solution
The hearing aid whistles continuously	Your ear is blocked by earwax	Contact your ENT doctor/physician
	The hearing aid is not correctly placed in your ear canal	Take the hearing aid out and reinsert it
	The hearing aid fits loosely in your ear canal	Contact your hearing care professional
The hearing aid is uncomfortable to wear	The hearing aid is not placed correctly in your ear canal	Consult your hearing care professional on how to place the hearing aid correctly in your ear canal.
	The hearing aid does not fit your ear properly	Contact your hearing care professional
	Your outer ear or ear canal is sore	Contact your hearing care professional

CARING FOR YOUR HEARING AID

The hearing aid is a valuable object and should be treated with care. Here are some things you can do to prolong the life of your hearing aid:

CAUTION

- Turn off your hearing aid when it is not in use. Remove the battery if the hearing aid will not be used for several days.
- When the hearing aid is not in use, keep it in its case in a dry location out of reach of children and pets.
- Do not expose the hearing aid to extreme temperatures or high humidity. Make sure to dry the hearing aid thoroughly after heavy perspiration such as that which may occur during intense physical activity, e.g. playing sports.
- Avoid dropping your hearing aid – perform cleaning and battery changes while holding the hearing aid above a soft surface.
- Do not wear your hearing aid while in the shower or swimming, or when using a hair dryer, perfume, hair and body sprays or gels such as suntanning lotions or creams.

WARNINGS

WARNING

Hearing aids and batteries can be dangerous if swallowed or used improperly. Swallowing or improper use can result in severe injury or even fatalities. In case of ingestion, contact a physician immediately.

- Keep hearing aids and their parts, accessories and batteries out of reach of children and anyone else who might swallow such items or otherwise cause injury to themselves. Do not change batteries in front of them and do not let them see where you keep your battery supply. Discard used batteries carefully.
- Batteries are very small and can easily be mistaken for pills or the like. Never put a battery or hearing aid in your mouth for any reason as you may risk swallowing it.
- Clean and inspect your hearing aid after use to check that it is intact. If the hearing aid breaks while in the ear canal, contact your hearing care professional immediately. Do not try to remove the parts yourself.

WARNING

- Risk of explosion if battery is replaced by an incorrect type or recharged. Dispose of used batteries according to the instructions.
- Never allow others to wear your hearing aid, as this could cause permanent damage to their hearing.
- When selecting a listening program, please remember that there are situations in which it is particularly important to be able to hear the surrounding sounds (e.g. traffic, warning signals).
- The hearing aid is made of modern non-allergenic materials. Nonetheless, in rare cases skin irritation may occur. If you notice skin irritation in or around your ear or ear canal, contact your hearing care professional.
- Please note that when using any type of hearing aid, you must allow regular ventilation of the ear. If the ear is not adequately ventilated, there may be a slightly increased risk of infection or disease in the ear canal. We therefore recommend that you remove the hearing aid from your ear when you go to bed, to allow the ear canal to be ventilated. If possible, you should also remove your hearing aid during the day if there are any periods when you do not need them. Make sure that you clean and inspect your hearing aid as required. If an ear infection or disease occurs, you should seek medical attention and contact your hearing care professional for advice on how to disinfect the hearing aid. Do not under any circumstances use alcohol, chlorine or similar substances for this purpose.

WARNING

- Regular use of a de-humidifier is recommended to help avoid malfunction of the hearing aid.
- Do not use Widex hearing aids in mines or other areas with explosive gases.

WARNING

- **Do not wear your hearing aid during radiation, X-rays, MRIs, CT or other medical treatments and scans.** The emissions from these procedures as well as from other types of radiation, such as that in a microwave oven, can damage your hearing aid and the hearing aid can become very hot. Radiation from, for example, room surveillance equipment, burglar alarms and mobile phones is weaker and will not damage the hearing aid, but may create audible interference.

CAUTION

- Your hearing aid has been tested for interference according to international standards. Nevertheless, it is possible that unforeseen interference may occur in the hearing aid due to electromagnetic radiation from other products such as alarm systems, room surveillance equipment and mobile phones.
- Although your hearing aid has been designed to comply with the most stringent international electromagnetic compatibility standards, the possibility cannot be excluded that it may cause interference with other equipment, such as medical devices.
- Never try to open or repair the hearing aid yourself.

ADVICE

NOTE

- The hearing aid will not restore normal hearing and will not prevent or improve a hearing loss resulting from organic conditions. However, the hearing aid can help you to make the best possible use of your remaining hearing ability. You should also bear in mind that it can take time to get used to a new hearing aid and new sounds.
- In most cases, using the hearing aid infrequently will not permit you to gain full benefit from it.
- The use of a hearing aid is only part of hearing habilitation and may need to be supplemented by auditory training and instruction in lipreading.
- The use of hearing aids increases the risk of accumulation of earwax. Contact your physician/ENT doctor if you suspect that a plug of earwax has accumulated in your ear. Earwax may not only reduce your own hearing but also the effect of the hearing aid considerably. It is a good idea to ask your physician to clean your ears a couple of times a year.

Electrical and electronic equipment (EEE) contains materials, components and substances that can be hazardous and present a risk to human health and the environment when waste electrical and electronic equipment (WEEE) is not handled correctly.

Do not dispose of hearing aids, hearing aid accessories and batteries with ordinary household waste.

Hearing aids, batteries and hearing aid accessories should be disposed of at sites intended for waste electrical and electronic equipment, or given to your hearing care professional for safe disposal. Proper disposal helps to protect human health and the environment.

SYMBOLS

Symbols commonly used by Widex A/S in medical device labelling (labels/IFU/etc.)

Symbol	Title/Description
	Manufacturer The product is produced by the manufacturer whose name and address are stated next to the symbol. If appropriate, the date of manufacture may also be stated.
	Date of manufacture The date when the product was manufactured.
	Use-by date The date after which the product is not to be used.
	Batch code The product's batch code (lot or batch identification).
	Catalogue number The product's catalogue (item) number.
	Serial number The product's serial number.*
	Keep away from sunlight The product must be protected from light sources and/or The product must be kept away from heat

Symbol	Title/Description
	Keep dry The product must be protected from moisture and/or The product must be kept away from rain
	Lower limit of temperature The lowest temperature to which the product can be safely exposed.
	Upper limit of temperature The highest temperature to which the product can be safely exposed.
	Temperature limits The highest and lowest temperatures to which the product can be safely exposed.
	Consult instructions for use The user instructions contain important cautionary information (warnings/precautions) and must be read before using the product.
	Caution/Warning Text marked with a caution/warning symbol must be read before using the product.
	WEEE mark **“Not for general waste”** When the product is to be discarded, it must be sent to a designated collection point for recycling and recovery.

Symbol	Title/Description
	CE mark The product is in conformity with the requirements set out in European CE marking directives.
	Alert The product is identified by R&TTE Directive 1999/5/EC as an equipment Class 2 product with some restrictions on use in some CE member states.
	C-Tick mark The product complies with EMC and radio spectrum regulatory requirements for products supplied to the Australian or New Zealand market.
	Interference Electromagnetic interference may occur in the vicinity of the product.

*The six- or seven-digit number on the product is the serial number. Serial numbers may not always be preceded by SN

WIDEX A/S Nymoellevej 6, DK-3540 Lynge, Denmark
www.widex.com

CE 0459

Manual no.:
9 514 0208 001 #03

9 514020 800102

WIDEX, MENU and NANOCARE are trademarks of Widex A/S

FSC
www.fsc.org
MIX
From responsible sources
FSC® C068122